


Humidity Difference to SHT85 average

[illegible]

v9_temperature_test0.CSV time: 17:54:37

SHT2X	SHT3X	SHT8X	SHTC1	SHTC3	BME280	Si7021	HTU21d	HDC1080	HDC2080	AM2320	AHT15	AHT20	CC2D33	HIH7120
-0.10	0.01	-0.03	-0.15	0.31	0.87	-0.29	0.09	0.02	0.43	-0.10	-0.77	-0.41	0.11	0.31
-0.14	0.02	-0.03	-0.21	0.28	0.70	-0.29	-0.08	0.30	0.53	-0.70	-0.63	-0.06	0.14	0.28
-0.04	-0.07	0.06	0.11		0.00	-0.04	-0.20	0.26	0.55	-0.40	-0.76	-0.82	0.10	
-0.13	-0.07		-0.13		0.39	-0.10	0.11	-0.23	0.62	-0.20	-0.74	-0.38		
0.01	-0.05		-0.16		0.07	-0.19	-0.11	-0.34	0.51	-0.50				
-0.02	-0.01					-0.13	-0.21	-0.30	0.56	-0.50				
-0.07	0.05					-0.07	0.02	-0.23	0.56	-0.50				
0.11	-0.03					0.15	0.09	-0.30	0.41	-0.10				
	-0.07													

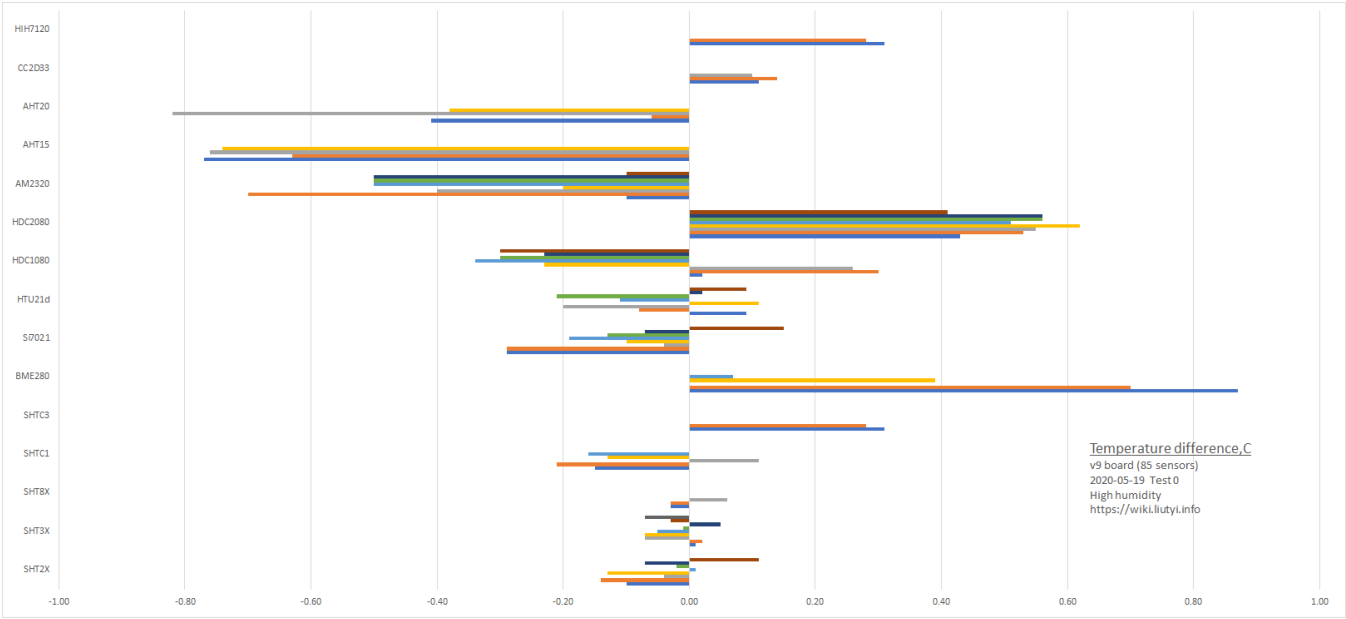

temperature overview

