

Test 5 v10b NaCl solution draft

That is supposed to be a Saturated NaCl solution that gives 75% RH, but this time SHT85 shows 77.7%. So it might be not perfect, also some AHT25 sensors got some weird numbers.

Humidity

H_1B_026.CSV

H_1B_027.CSV


Measurement for time 23:12

HIH7120	SHT85	AHT10	AHT20	AHT21	AHT25
80.31	77.67	79.59	77.81	75.67	89.03
		80.04	78.91	74.33	85.72
		79.42	78.83	74.71	85.48
		80.89	79.79	79.81	96.34
		78.44	78.22	72.7	88.75
		78.3	82.25	77.7	90.07
		77.78	79.39	74	79.25
		79.83	81.12	74.93	90.45
80.31	77.67	79.29	79.54	75.48	88.14

Average measurement for time 23:12

HIH7120	SHT85	AHT10	AHT20	AHT21	AHT25
80.31	77.67	79.29	79.54	75.48	88.14

Humidity trend

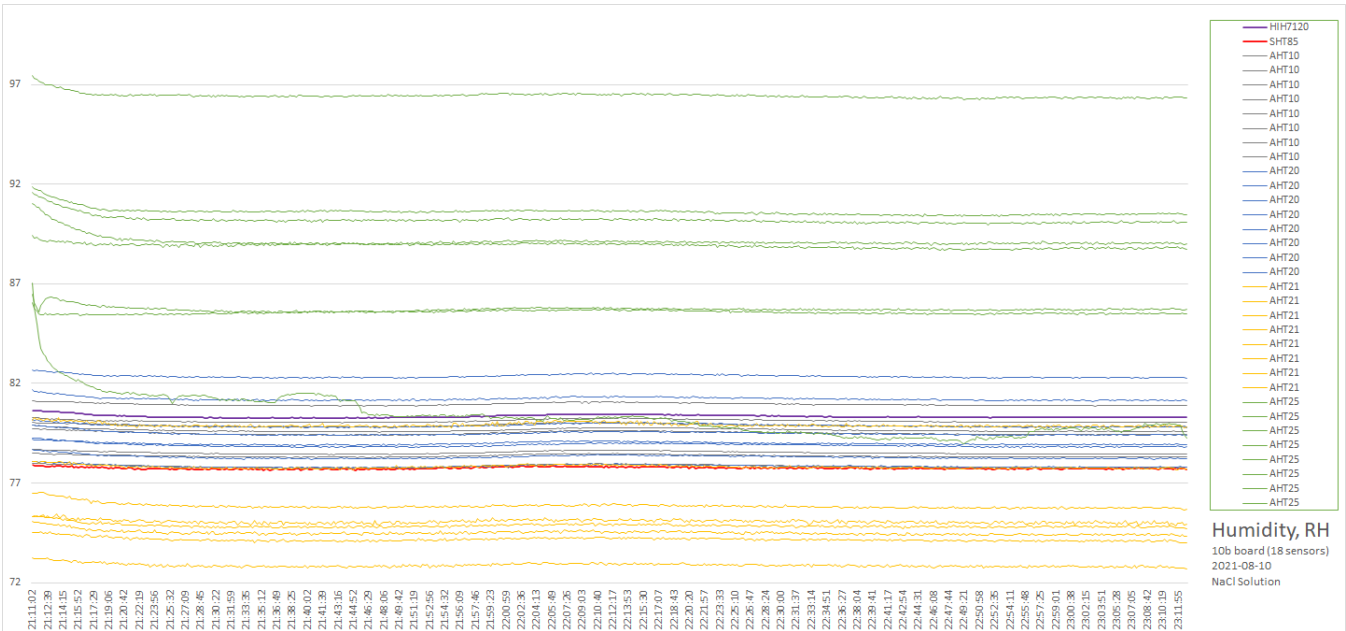

Temperature

T_1B_026.CSV

T_1B_027.CSV

Measurement for time 23:12

HIH7120	SHT85	AHT10	AHT20	AHT21	AHT25
27.3	27.34	27.56	26.8	27.09	27.52
		27.18	26.91	27.35	27.62
		27.25	26.89	27.05	27.89
		27.29	27.01	27.47	27.95
		27.24	26.89	27.06	27.84
		27.28	26.83	26.8	27.59
		27.46	26.81	27.21	29.08
		27.23	27.28	27.09	27.69
27.30	27.34	27.31	26.93	27.14	27.90

Average measurement for time 23:12

HIH7120	SHT85	AHT10	AHT20	AHT21	AHT25
27.30	27.34	27.31	26.93	27.14	27.90

Temperature trend

