

# Test 4 v10b Freezer 1 draft

## Humidity

H\_1B\_023.CSV


Measurement for time 23:00

| HIH7120 | SHT85 | AHT10 | AHT20 | AHT21 | AHT25 |
|---------|-------|-------|-------|-------|-------|
| 65.63   | 62.68 | 55.04 | 48.12 | 61.09 | 64.9  |
|         |       | 54.69 | 54.16 | 57.62 | 59.97 |
|         |       | 57.26 | 58.01 | 55.2  | 62.68 |
|         |       | 49.84 | 49.88 | 58.8  | 66.7  |
|         |       | 51.34 | 54.23 | 54.95 | 63.77 |
|         |       | 48.32 | 53.17 | 57.35 | 62.41 |
|         |       | 54.31 | 60.35 | 58.12 | 56.73 |
|         |       | 55.94 | 56.12 | 67.12 | 62.42 |
| 65.63   | 62.68 | 53.34 | 54.26 | 58.78 | 62.45 |


Average measurement for time 23:00

| HIH7120 | SHT85 | AHT10 | AHT20 | AHT21 | AHT25 |
|---------|-------|-------|-------|-------|-------|
| 65.63   | 62.68 | 53.34 | 54.26 | 58.78 | 62.45 |

## Humidity trend overview

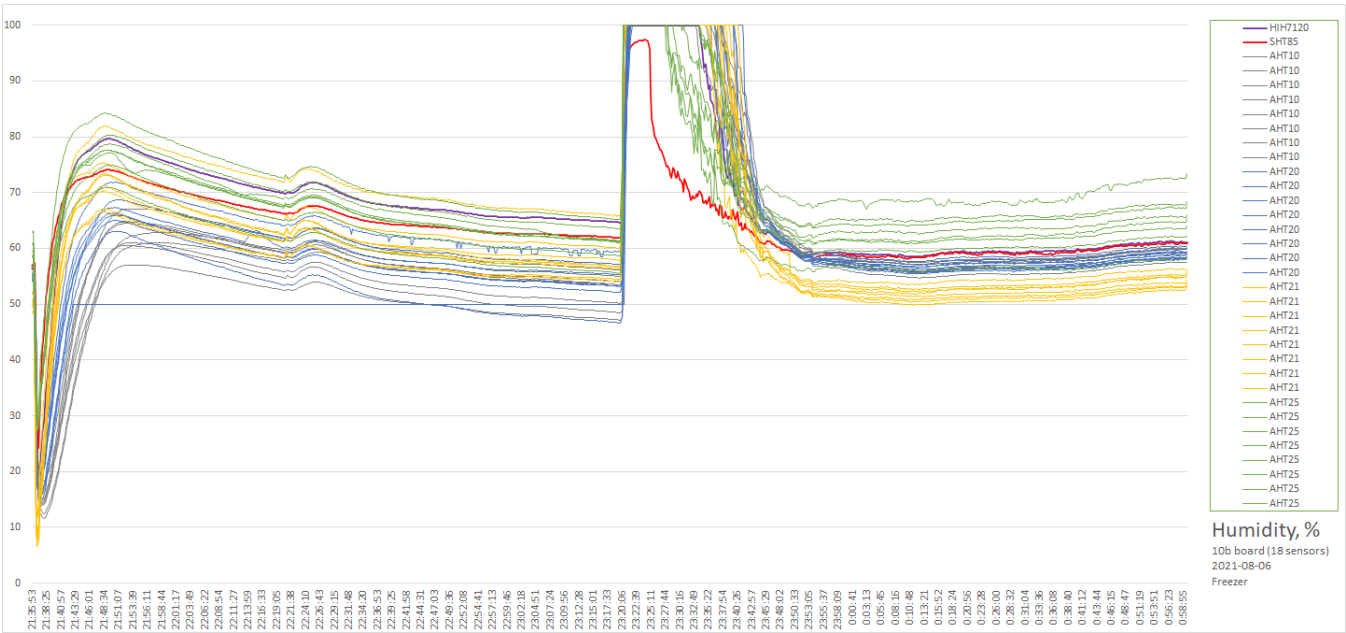

## Humidity trend fragment

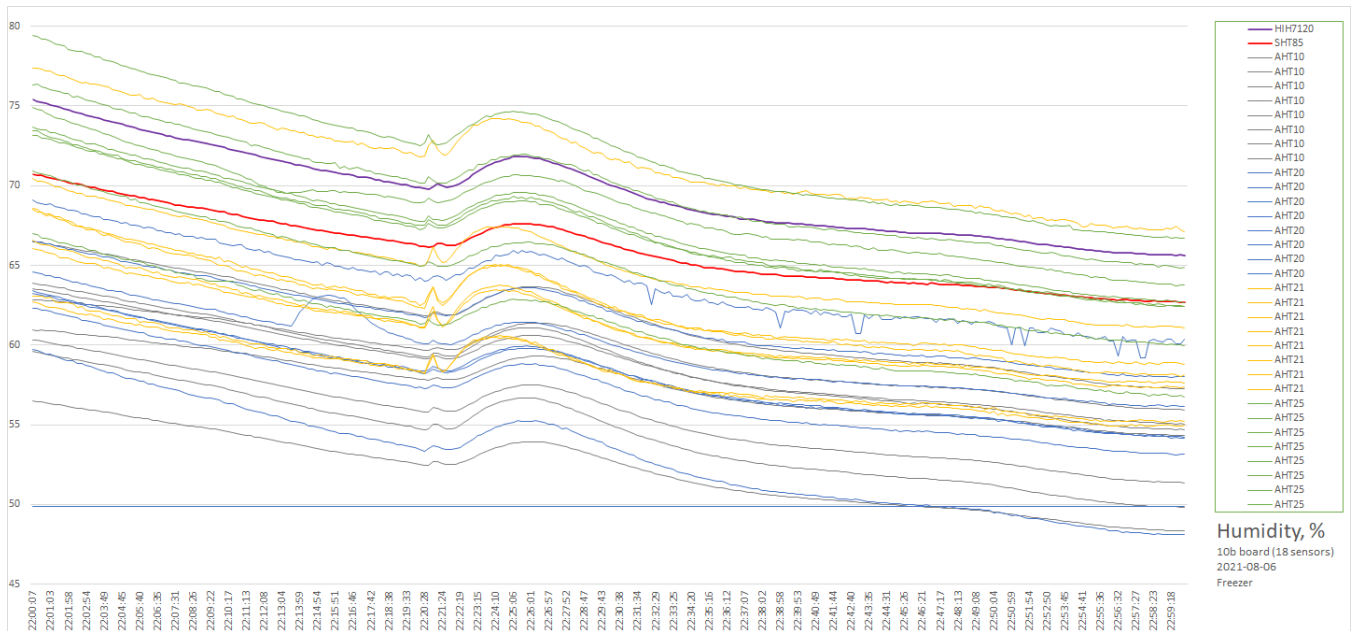

# Temperature

T\_1B\_023.CSV


Measurement for time 23:00

| HIH7120 | SHT85  | AHT10  | AHT20  | AHT21  | AHT25  |
|---------|--------|--------|--------|--------|--------|
| -20.44  | -22.9  | -23.88 | -23.52 | -23.65 | -16.11 |
|         |        | -23.16 | -25.46 | -22.9  | -16.55 |
|         |        | -25.01 | -25.36 | -24.1  | -17.38 |
|         |        | -24.24 | -17.48 | -25.5  | -17.22 |
|         |        | -23.67 | -25.27 | -24.48 | -16.91 |
|         |        | -23.37 | -24.25 | -23.69 | -17.11 |
|         |        | -25.39 | -25.29 | -23.8  | -16.04 |
|         |        | -22.7  | -27.11 | -23.36 | -16    |
| -20.44  | -22.90 | -23.93 | -24.22 | -23.94 | -16.67 |

Average measurement for time 23:00

| HIH7120 | SHT85  | AHT10  | AHT20  | AHT21  | AHT25  |
|---------|--------|--------|--------|--------|--------|
| -20.44  | -22.90 | -23.93 | -24.22 | -23.94 | -16.67 |

## Temperature trend overview

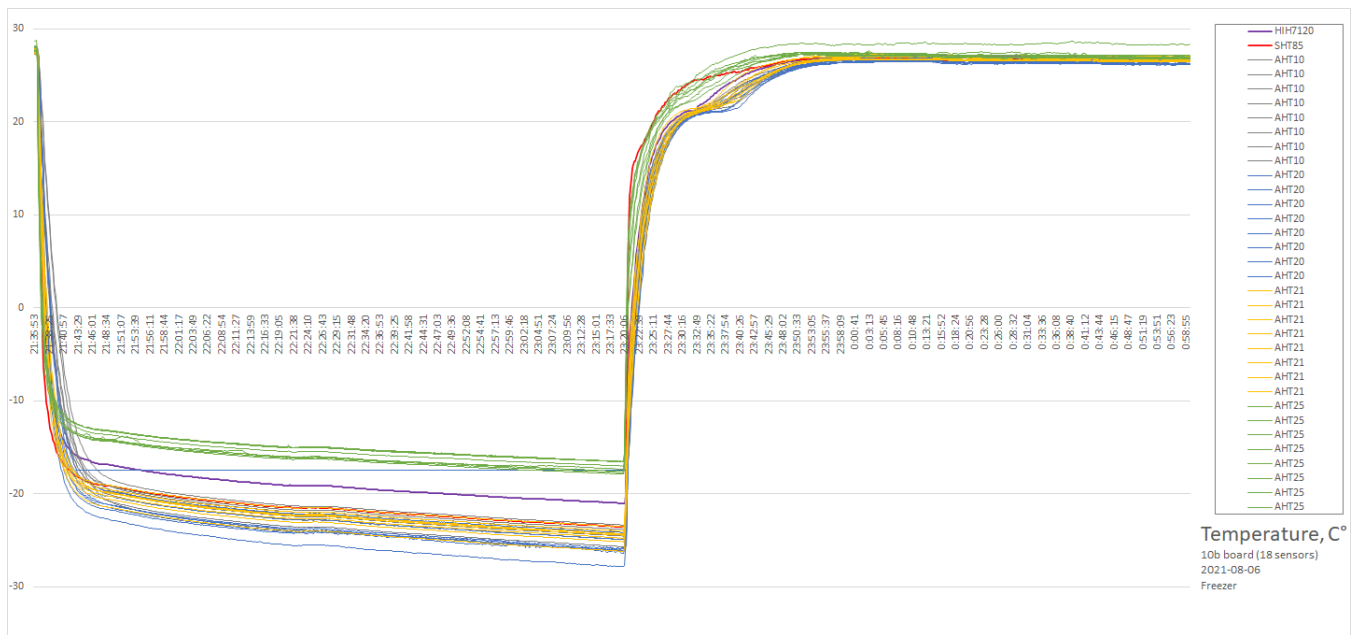

Temperature trend fragment

